

Transaction Information

Tool ID	QRE015
Tool Status	Disconnected
Location	Dresden, Germany
Wafer Size	NA
Fab Section	Reliability Lab,
Tool Available Date	2025-03-03

General Product Information

Vendor Supplier	AETRIUM
Model	1164 Reliability Test System
Vintage	2004
Serial No	150
Asset Description	Reliability Package level tester (multiple)
Software Version	n/a
CIM	none
Process	Lab Analysis

Hardware Configuration

System Type	Description	Quantity	Status
Main System	Mainframe / TCU	1	OK
Handler System	N/A		
Factory Interface	NONE		
Options System	-		
Others	-		
Main System			OK

Excluded Items List (Pumps, Chillers & Abatement are all excluded)

Description	Quantity

* List above may or may not be comprehensive. Tool is sold in "as-is" condition. To ensure your satisfaction, we strongly recommend to make an appointment to inspect this and every tool you are interested in.

Tool Pictures

General

NONE




General

NONE








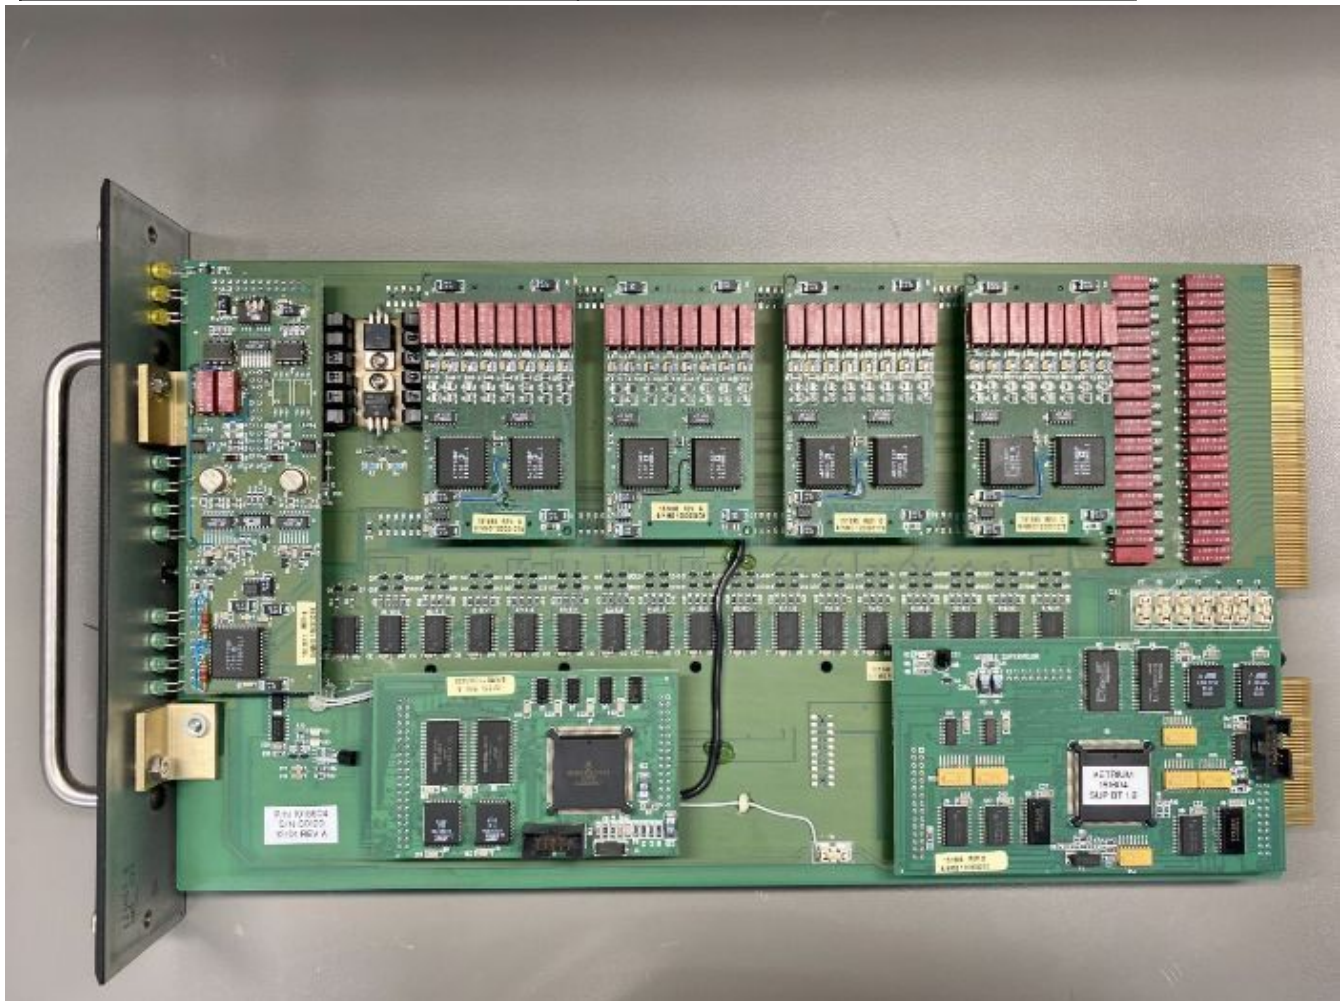


Hardware Fab

NONE

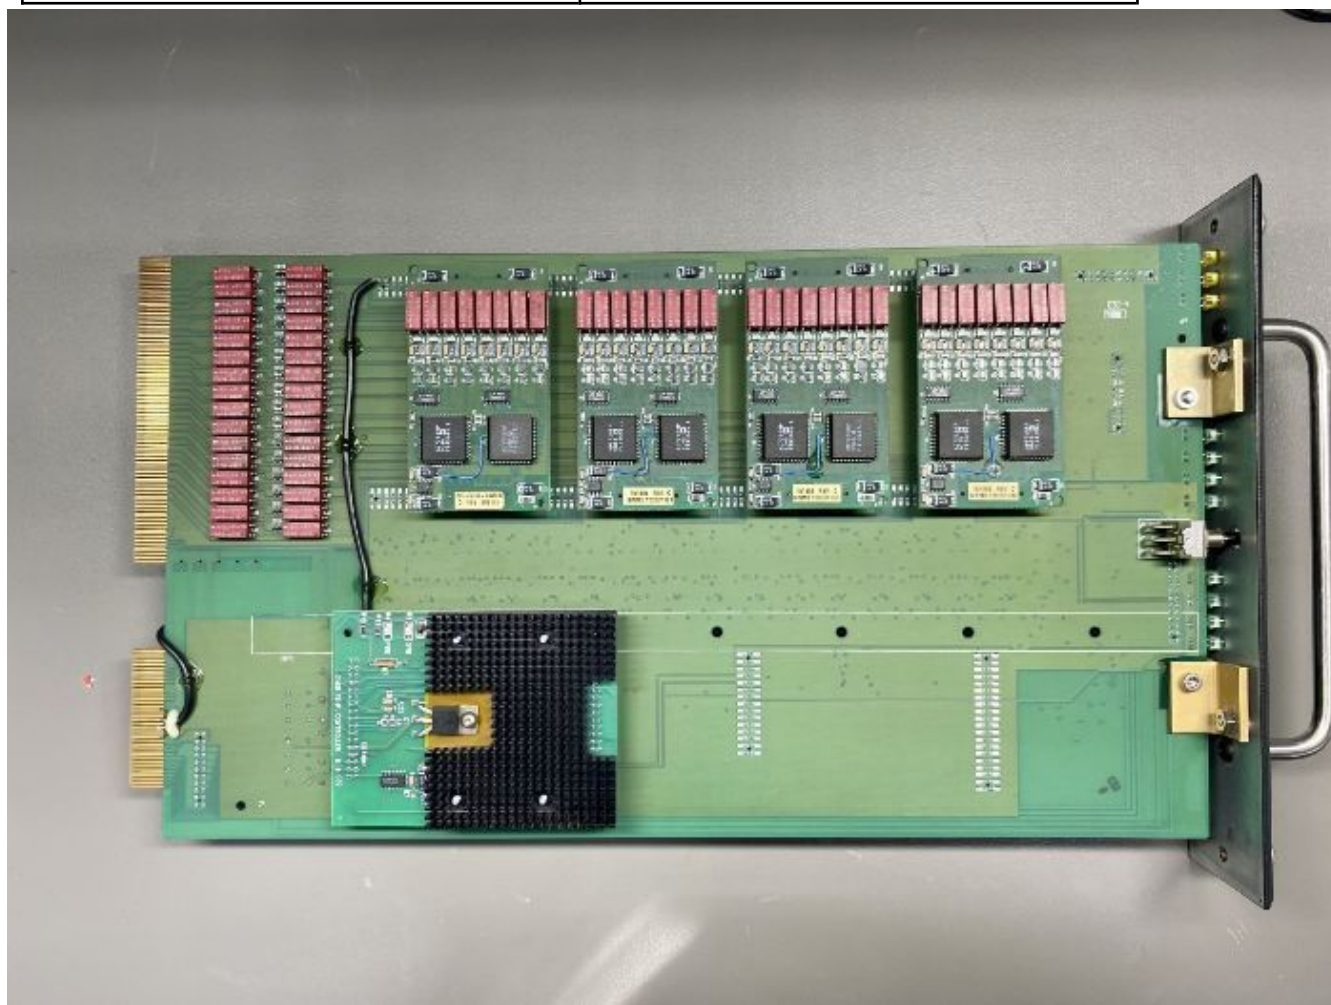


Hardware Fab

NONE

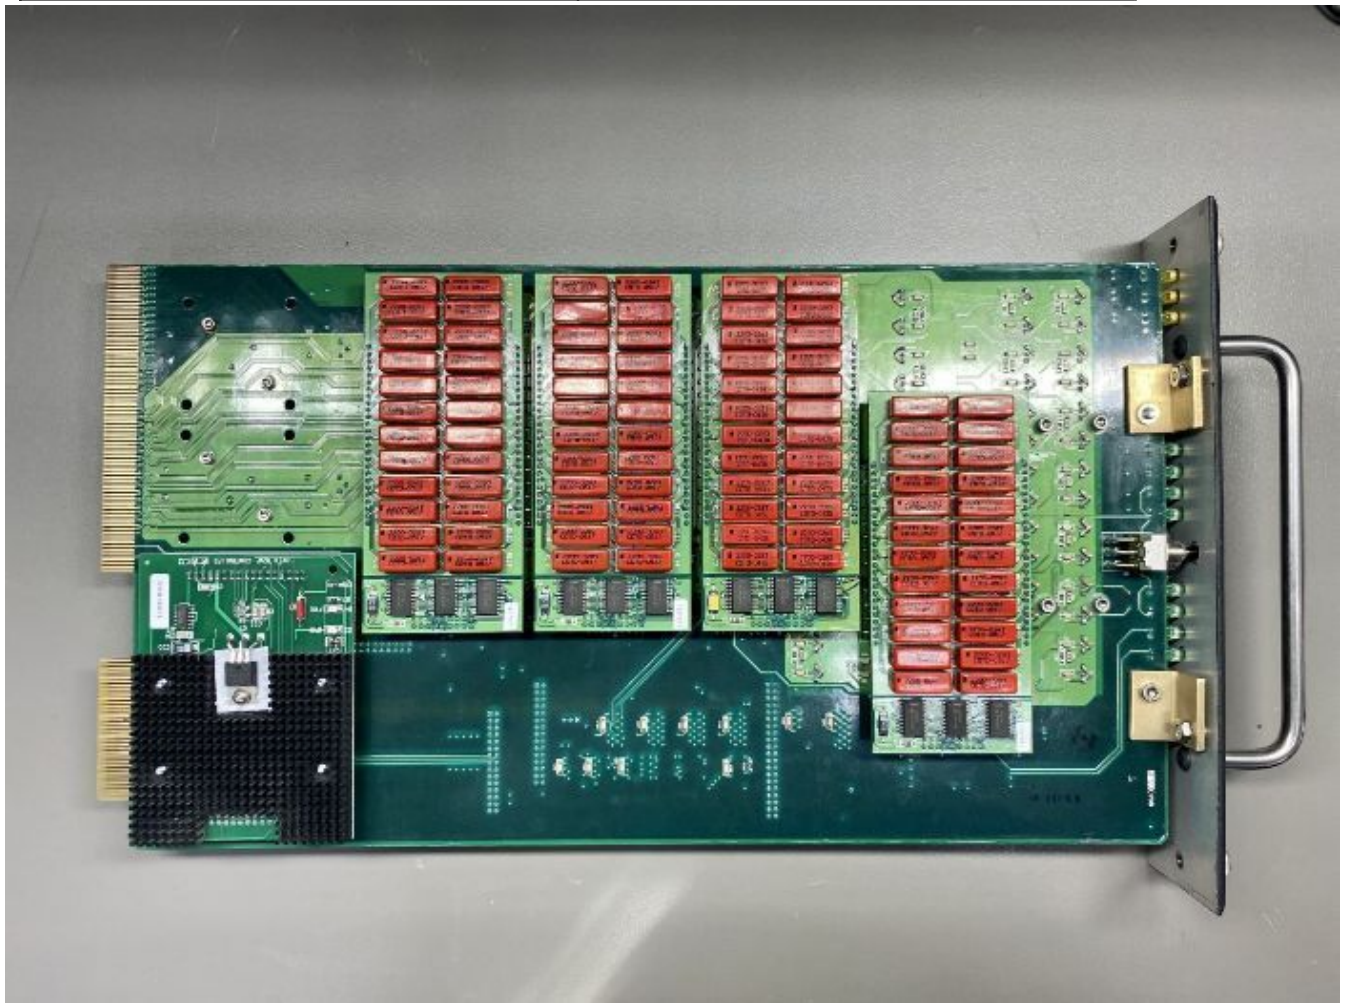

Hardware Fab

NONE

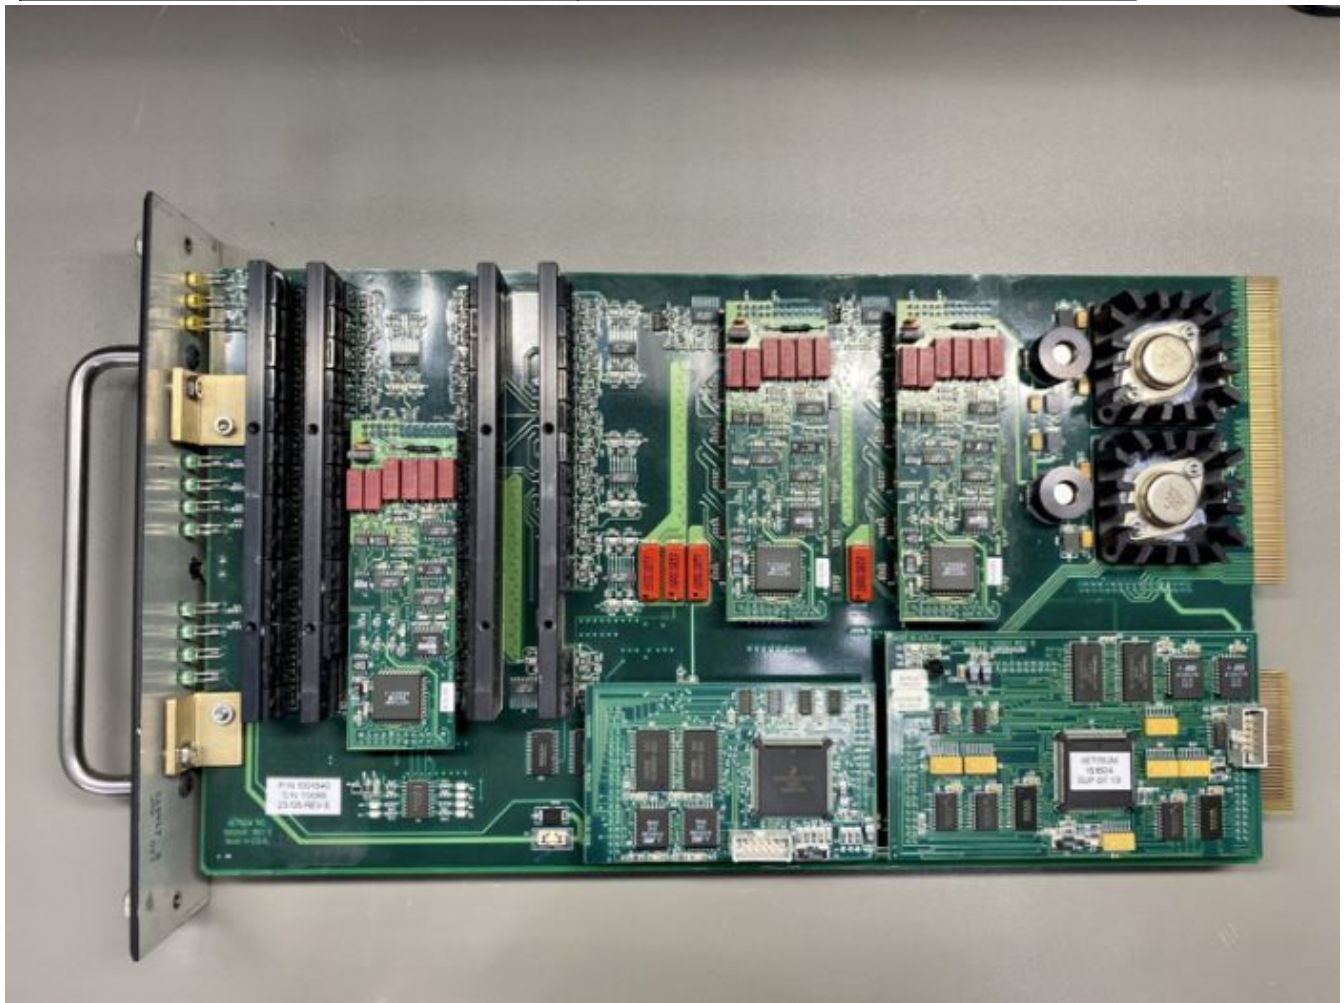

Manufacture Serial

NONE

